



Calibración para 5KV

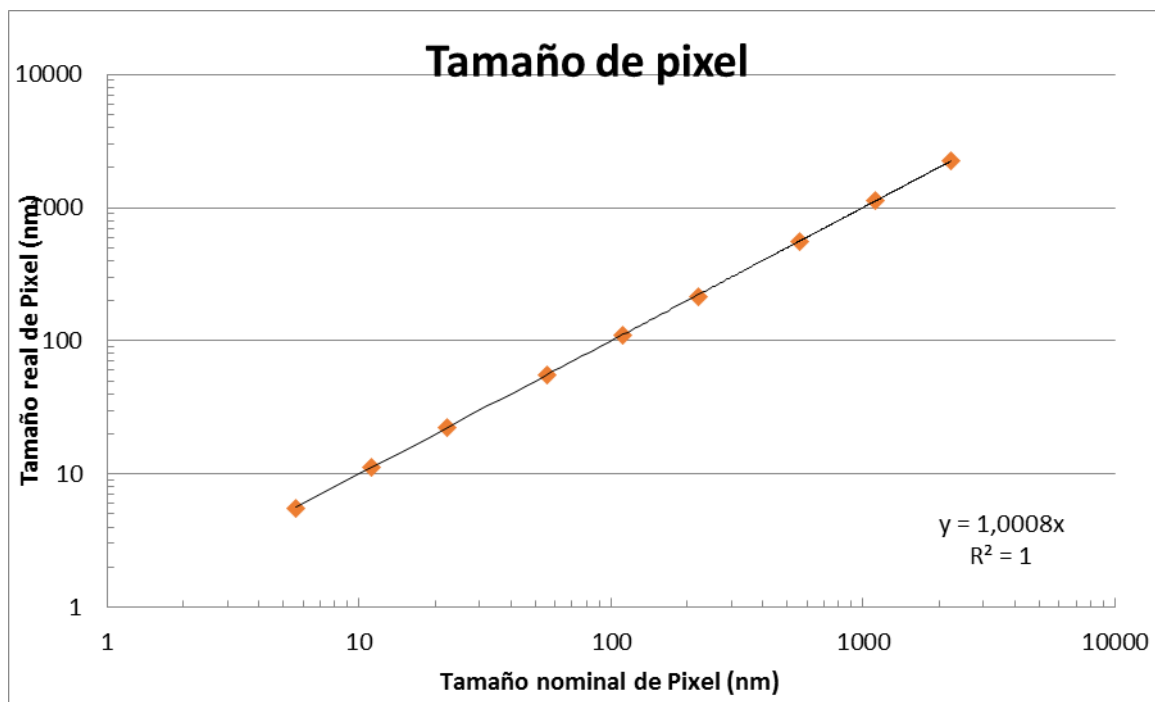


$$P_{\text{real}} = (1,001 \pm 0,001) P_{\text{nominal}}$$

$$r^2 = 0,999998$$

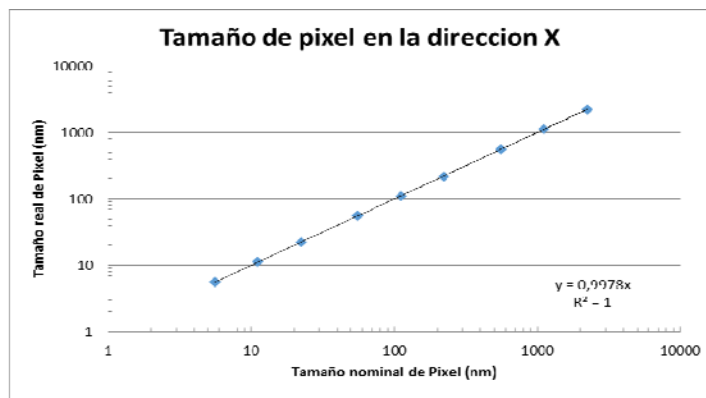

$$P_{X_{\text{real}}} = (0,998 \pm 0,001) P_{X_{\text{nominal}}}$$

$$r^2 = 0,999990$$

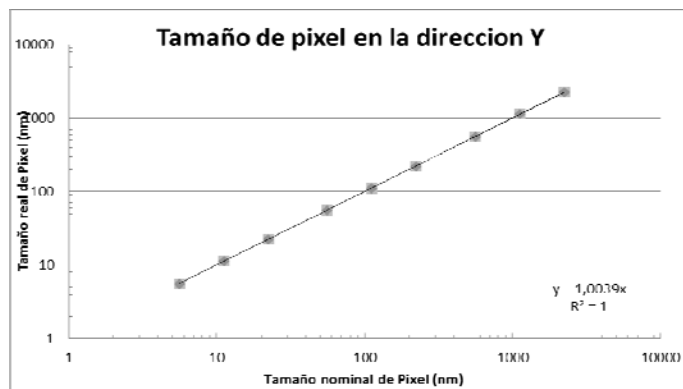


$$P_{Y_{\text{real}}} = (1,003 \pm 0,001) P_{Y_{\text{nominal}}}$$

$$r^2 = 0,99998$$


Calibración realizada por Francisco Varela el 2021/02/15

Calibración para 10KV

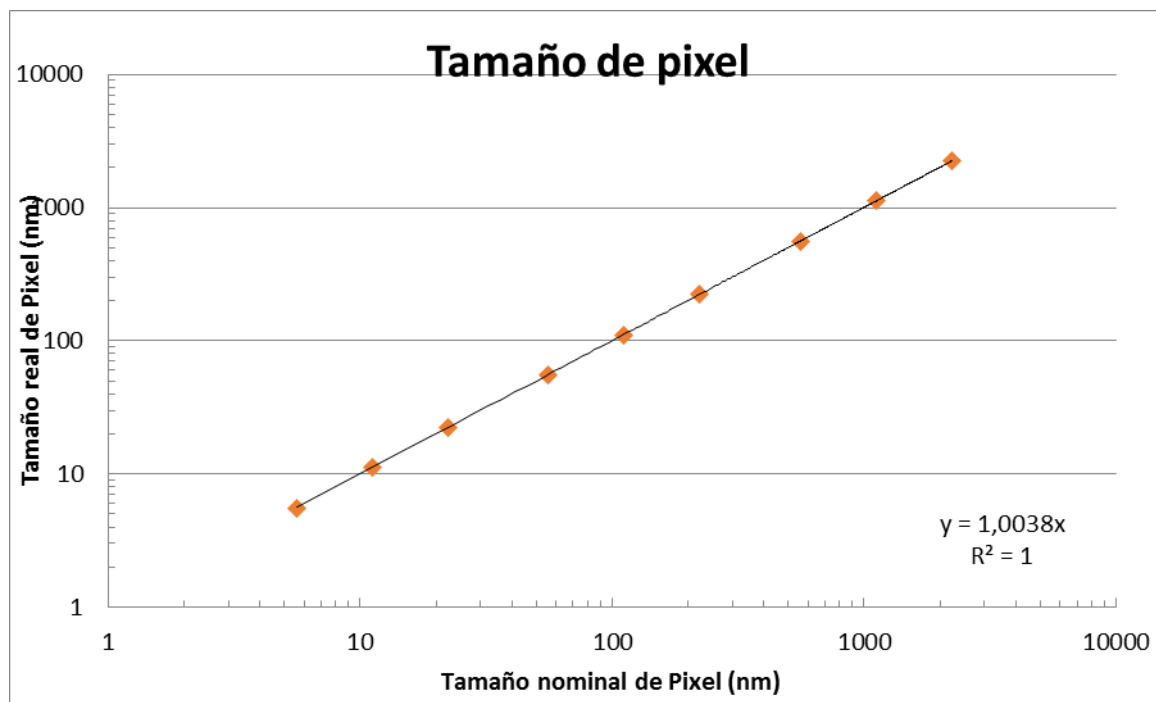


$$P_{\text{real}} = (1,0038 \pm 0,0010) P_{\text{nominal}}$$

$$r^2 = 0,999991$$

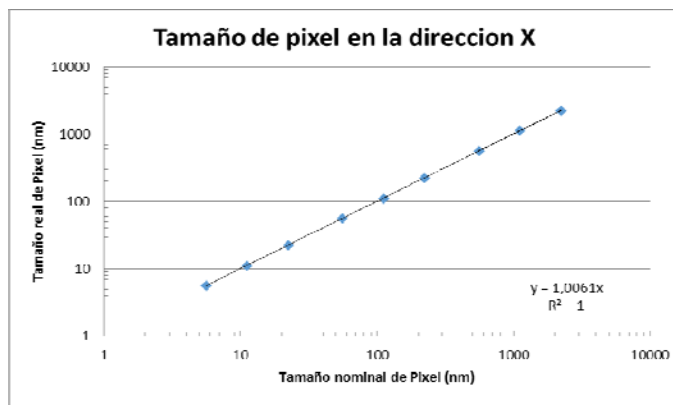

$$P_{X\text{real}} = (1,0061 \pm 0,001) P_{X\text{nominal}}$$

$$r^2 = 0,99998$$

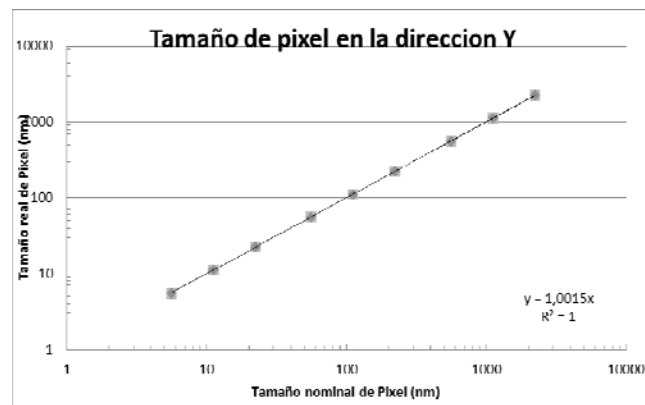


$$P_{Y\text{real}} = (1,0015 \pm 0,0009) P_{Y\text{nominal}}$$

$$r^2 = 0,999993$$


Calibración realizada por Francisco Varela el 2021/02/15

Calibración para 20KV

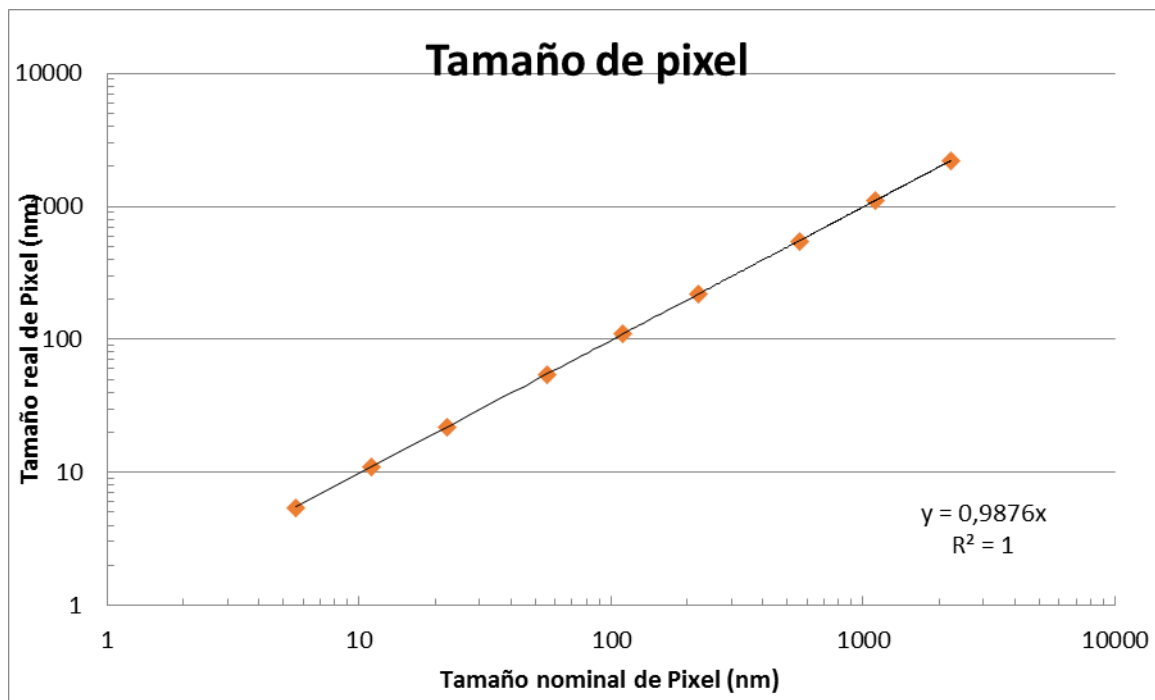


$$P_{\text{real}} = (0,987 \pm 0,001) P_{\text{nominal}}$$

$$r^2 = 0.999997$$

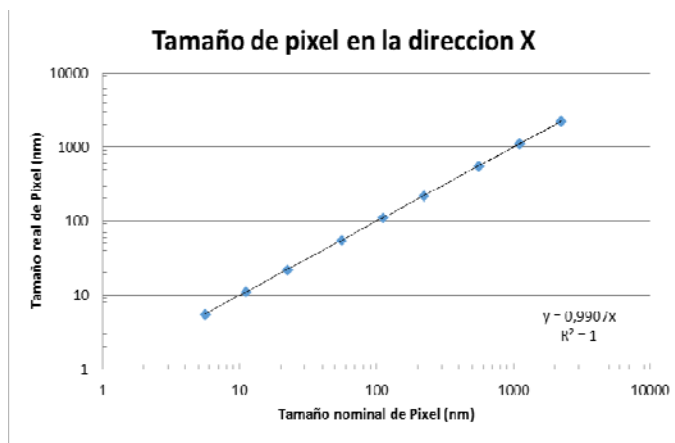

$$P_{X\text{real}} = (0,991 \pm 0,001) P_{X\text{nominal}}$$

$$r^2 = 0,99998$$

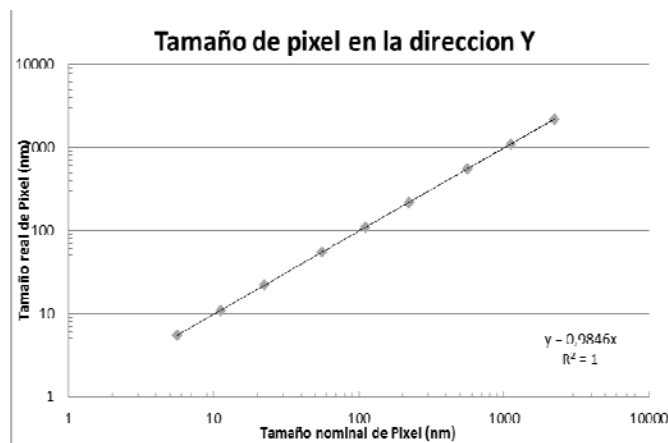


$$P_{Y\text{real}} = (0,9846 \pm 0,0004) P_{Y\text{nominal}}$$

$$r^2 = 0,999998$$


Calibración realizada por Francisco Varela el 2021/02/15

Calibración para 30KV

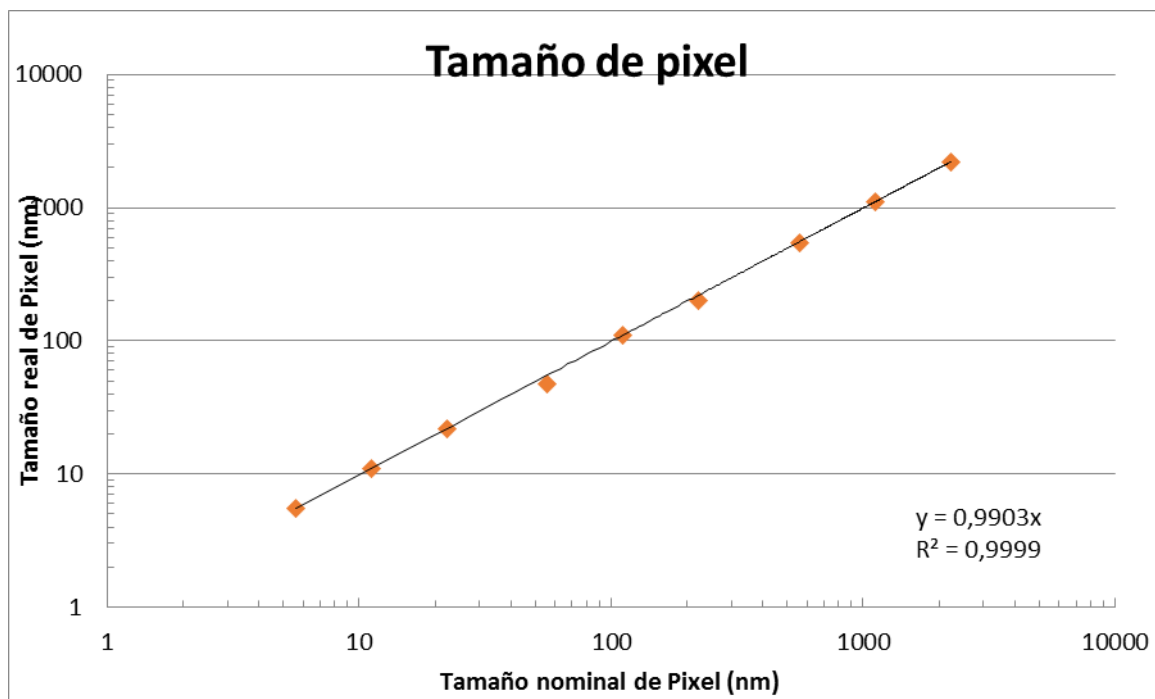


$$P_{\text{real}} = (0,990 \pm 0,003) P_{\text{nominal}}$$

$$r^2 = 0,99991$$

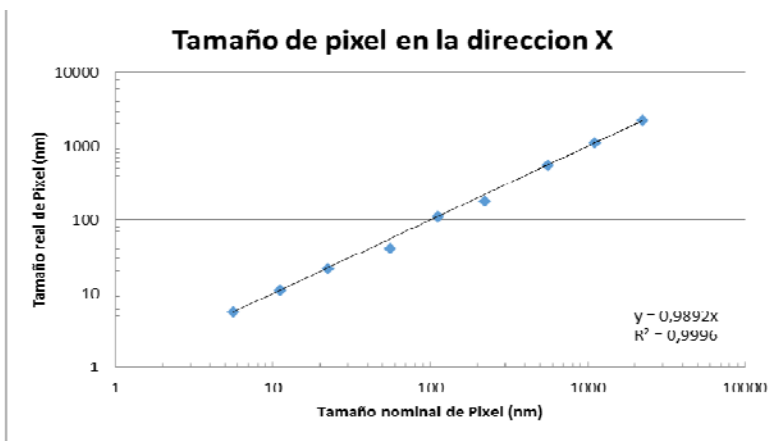

$$P_{X\text{real}} = (0,989 \pm 0,006) P_{X\text{nominal}}$$

$$r^2 = 0,9997$$

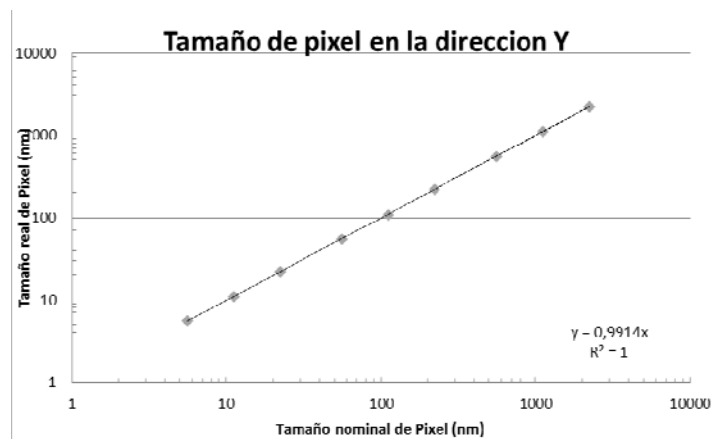

$$P_{Y\text{real}} = (0,991 \pm 0,001) P_{Y\text{nominal}}$$

$$r^2 = 0,99998$$

Calibración realizada por Francisco Varela el 2021/02/15